


# ordering information

A complete range with a variety of lengths


Reference	Diameter (mm)	Length (cm)	Box unit content
SPIF2,5x5P10	2,5	5	5
SPIF2,5x10P10	2,5	10	5
SPIF2,5x20P10	2,5	18,5	5

Spif flow coils

## spif compatibilities




**Magic**  
1,2F & 1,5F & 1,8F



**Sonic**  
1,2F & 1,5F



**Baltacci**  
1,2F & 1,5F & 1,8F



**Vasco+**  
10 & 18 & 21

\*Arteriovenous malformation

\*\*Chapot et al., (2014) The Pressure Cooker Technique for the treatment of brain AVMs

The occlusion devices Flow Coils are intended for the embolization of vascular malformations of the vasculature. Class III CE0297 in compliance with Medical Device Directive (MDD 93/42/EEC amended by 2007/47/EC). Manufactured by BALT EXTRUSION SAS. Carefully read the instructions for use before use. French reimbursement codes 3123690. First CE marking:2008. MAGIC is a microcatheter intended for selective and hyperselective vascular catheterization for diagnostic and therapeutic purposes. Class III CE0297 in compliance with Medical Device Directive (MDD 93/42/EEC amended by 2007/47/EC). Manufactured by BALT EXTRUSION SAS. Carefully read the instructions for use before use. Not reimbursed. First CE marking:1998. SONIC is a braided microcatheter intended for selective and hyper selective vascular catheterization for diagnostic and therapeutic purposes. Class III CE0297 in compliance with Medical Device Directive (MDD 93/42/EEC amended by 2007/47/EC). Manufactured by BALT EXTRUSION SAS. Carefully read the instructions for use before use. Not reimbursed. First CE marking:2005. VASCO+ is a reinforced microcatheter intended for injection or diagnostic or therapeutic products; to position pushable coils "SPIRALES" or detachable coils especially the ones of MDS "mechanical detachment system"; for the use of the self-expanding stent LEO+ or SILK+. Class III CE0297 in compliance with Medical Device Directive (MDD 93/42/EEC amended by 2007/47/EC). Manufactured by BALT EXTRUSION SAS. Carefully read the instructions for use before use. Not reimbursed. First CE marking:2004. BALTACCI microcatheter is intended for selective and hyperselective vascular catheterization for diagnostic and therapeutic purposes. Class III CE0297 in compliance with Medical Device Directive (MDD 93/42/EEC amended by 2007/47/EC). Manufactured by BALT EXTRUSION SAS. Carefully read the instructions for use before use. Not reimbursed. First CE marking:1998. The content of this document, in particular data, information, trademarks and logo is BALT SAS and affiliates' sole property. ©2020 BALT SAS and affiliates, all rights reserved. All representation and/or reproduction, whether in part or in full, is forbidden and would be considered a violation of BALT SAS and affiliates' copyrights and other intellectual property rights. This document with associated pictures is non contractual and is solely dedicated to healthcare professionals and BALT's distributors (BALT's supplier's distributors). The products commercialized by BALT shall exclusively be used in accordance with the instructions for use included in the box. DC046GB (06/2020)

Balt

10, rue de la Croix Vigneron, 95160 Montmorency, France

Tél. : +33 (0)1 39 89 46 41


Fax : +33 (0)1 34 17 03 46

[www.balt-corp.com](http://www.balt-corp.com)



# flow coil

the free spirales compatible  
with 1,2F microcatheter

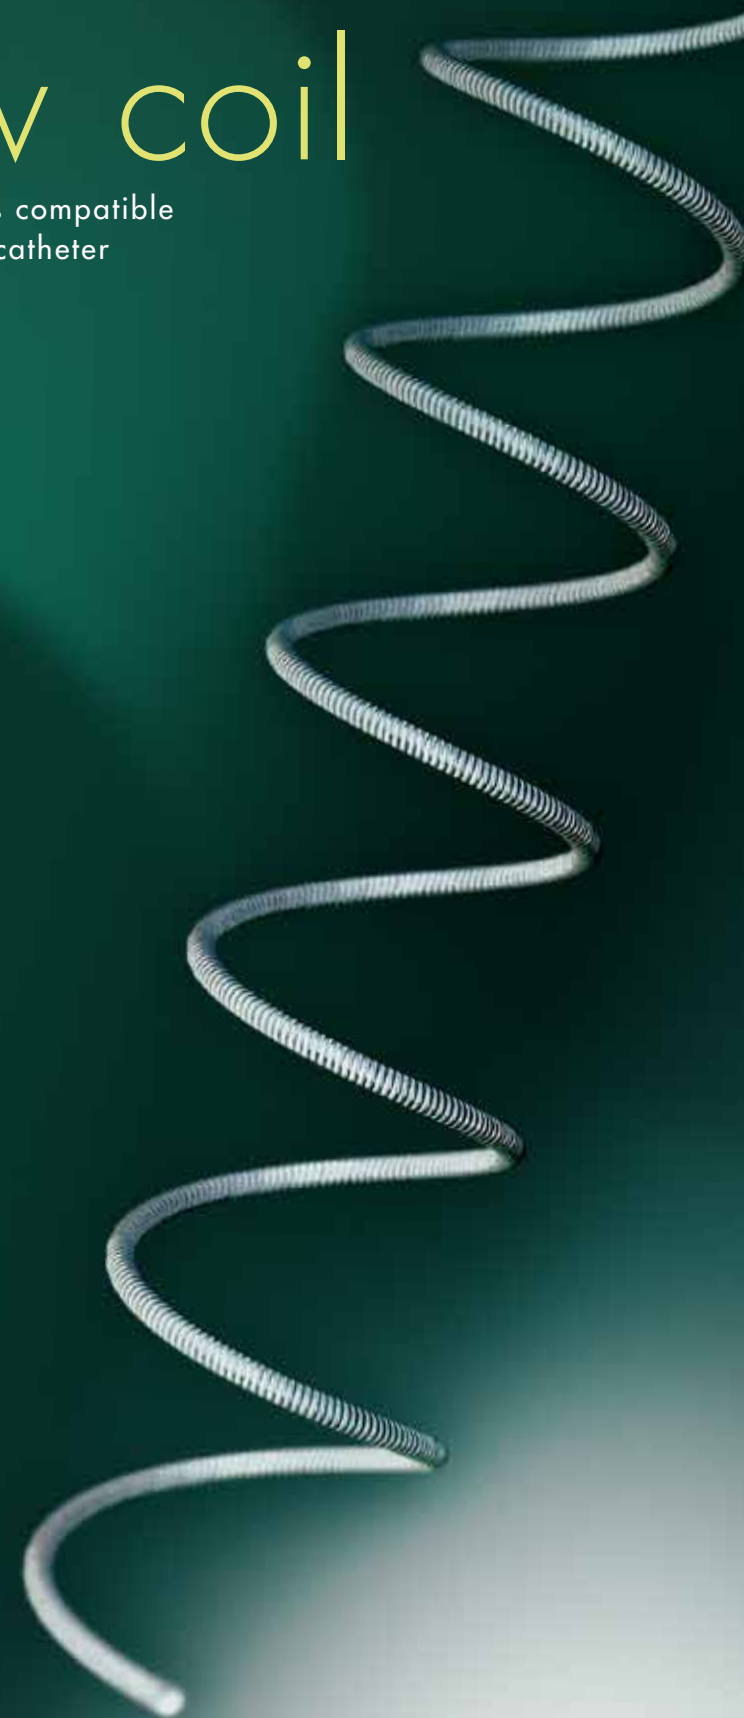

# flow coils

Free spirales for injection

Intended for the embolization of vascular malformation

.007" O.D.

avm\*  
treatment




.007"

- Unique compatibility thanks to its soft platinum radiopaque structure, to be injected through:
  - Magic 1,2F microcatheter
  - Sonic 1,2F microcatheter


## Pressure cooker technique

The Pressure Cooker Technique for the treatment of brain AVMs\*\* (Chapot et al., 2014)


- Sonic detachable tip
- Spif
- Distal marker of Magic 1,2F

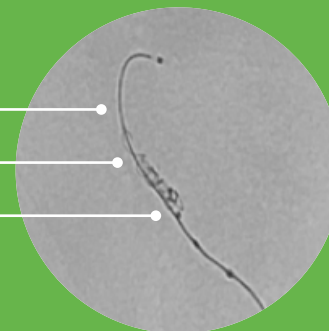

- Glue & Spif

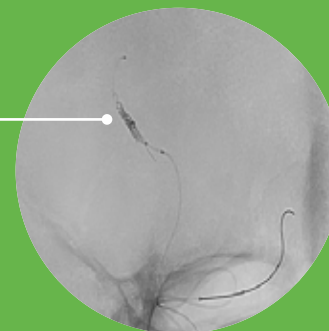

- Liquid embolic

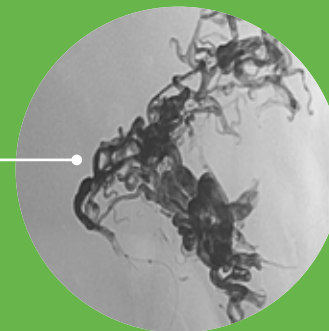

a unique  
compatibility  
with magic 1,2F